

Applicant(s): Frederick Geheb

CARDIO-PULMONARY RESUSCITATION DEVICE WITH
FEEDBACK FROM MEASUREMENT OF PULSE AND/OR
BLOOD OXYGENATION

FIGURE 1


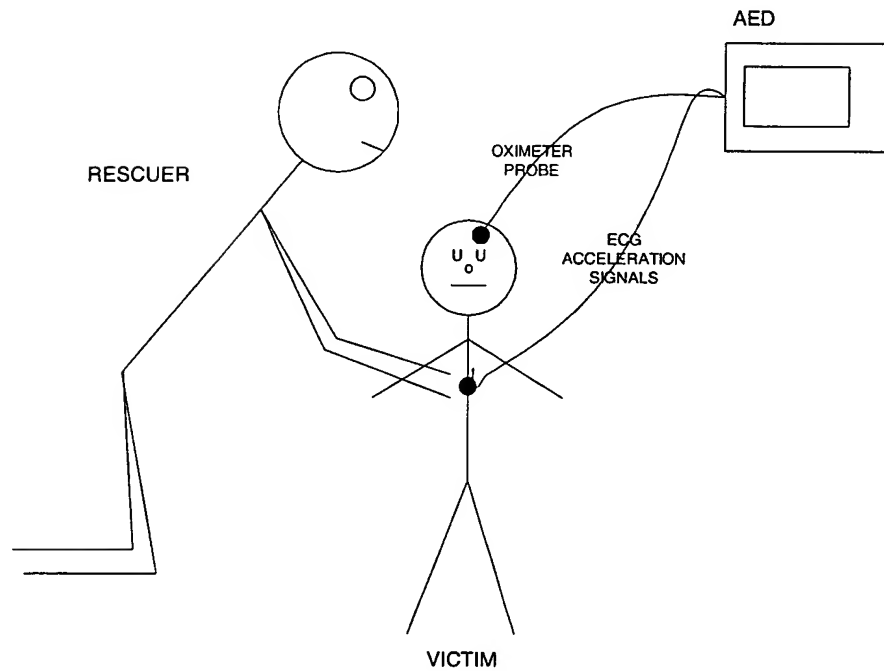


FIGURE 2

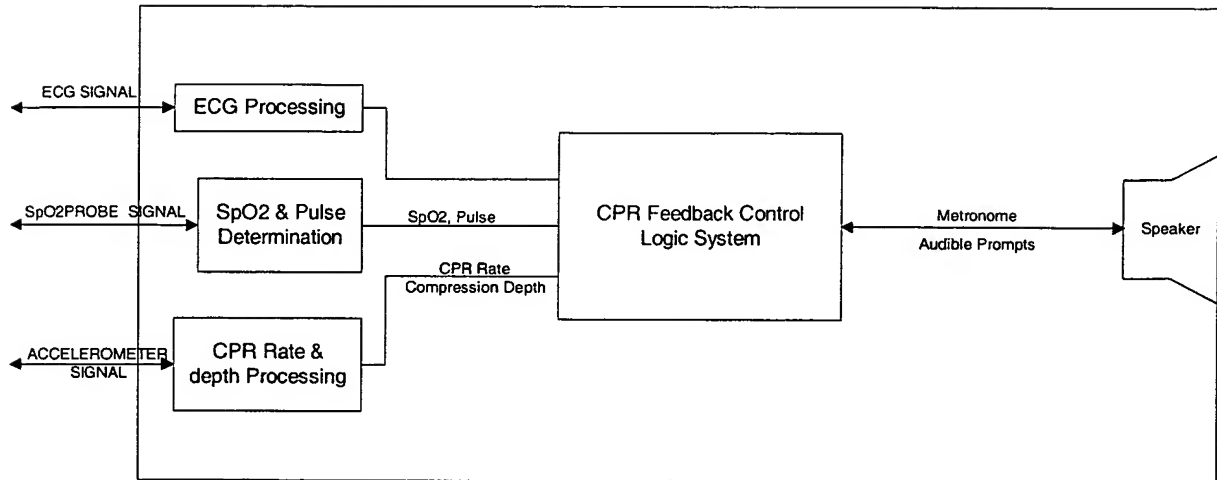

Applicant(s): Frederick Geheb

CARDIO-PULMONARY RESUSCITATION DEVICE WITH
FEEDBACK FROM MEASUREMENT OF PULSE AND/OR
BLOOD OXYGENATION**FIGURE 3**